



LAWRENCE
LIVERMORE
NATIONAL
LABORATORY

Spectroscopic diagnostics for liquid lithium divertor studies on the NSTX

V. A. Soukhanovskii, A. L. Roquemore, R. E. Bell,
R. Kaita, H. W. Kugel

June 7, 2010

Review of Scientific Instruments

Disclaimer

This document was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor Lawrence Livermore National Security, LLC, nor any of their employees makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or Lawrence Livermore National Security, LLC. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or Lawrence Livermore National Security, LLC, and shall not be used for advertising or product endorsement purposes.

Spectroscopic diagnostics for liquid lithium divertor studies on NSTX^{a)}

V. A. Soukhanovskii,^{1, b)} A. L. Roquemore,² R. E. Bell,² R. Kaita,² and H. W. Kugel²

¹⁾*Lawrence Livermore National Laboratory, Livermore, California*

²⁾*Princeton Plasma Physics Laboratory, Princeton, New Jersey*

The use of lithium-coated plasma facing components for plasma density control is studied in the National Spherical Torus Experiment. A recently installed liquid lithium divertor (LLD) module has a porous molybdenum surface, separated by a stainless steel liner from a heated copper substrate. Lithium is deposited on the LLD from two evaporators. Two new spectroscopic diagnostics are installed to study the plasma surface interactions on the LLD: 1) A 20-element AXUV diode array with a 6-nm bandpass filter centered at 121.6 nm (the Lyman- α transition) for spatially-resolved divertor recycling rate measurements in the highly-reflective LLD environment, and 2) An ultraviolet-visible-near infrared $R = 0.67$ m imaging Czerny-Turner spectrometer for spatially-resolved divertor D I, Li I-III, C I-V, Mo I, D₂, LiD, CD₄ emission and temperature measurements on and around the LLD module. The use of photometrically calibrated measurements together with atomic physics factors enables studies of recycling and impurity particle fluxes as functions of LLD temperature, ion flux, and divertor geometry.

Keywords: ultraviolet, visible, near infrared, spectroscopy, lithium, divertor, recycling

^{a)}Contributed paper, published as part of the Proceedings of the 18th Topical Conference on High-Temperature Plasma Diagnostics, Wildwood, New Jersey, USA, May 2010.

^{b)}Electronic mail: vlad@llnl.gov

I. INTRODUCTION

The use of lithium coatings evaporated on graphite plasma facing components (PFCs) has been under investigation for plasma density control and performance improvements in the National Spherical Torus Experiment (NSTX)^{1,2}. Recently, a liquid lithium toroidal module was installed in the NSTX lower divertor area. The liquid lithium divertor (LLD) module has a porous molybdenum surface, separated by a stainless steel liner from a copper substrate³. Lithium is deposited on the LLD surface from two overhead evaporators¹. A perceived advantage of the LLD over the solid lithium coating is a self-regenerating lithium surface for pumping hydrogenic fuel ions and atoms.

In order to assess the relationship between lithium-coated and liquid lithium divertor surface conditions and edge-core plasma transport and radiation properties, the NSTX diagnostics complex has been augmented with a new array of divertor Langmuir probes at the LLD radial location⁴, a material analysis and particle probe, a two color infrared thermography system⁵, and a charge-exchange recombination spectroscopy system⁶ upgraded for core lithium density measurements. In this paper we describe two new divertor diagnostics that are being installed on NSTX: (1) A Lyman- α (Ly_α) diode array (hereforth referred to as LADA) for divertor recycling measurements, and (2) A ultraviolet-visible-near infrared (UV-VIS-NIR) divertor imaging spectrometer (hereforth referred to as DIMS) for divertor atomic and molecular flux measurements. These diagnostics will contribute to the planned studies of retention and recycling of deuterium as a function of LLD surface conditions (e.g., Li coverage, temperature), divertor T_e and n_e , strike point proximity and flux expansion, as well as to relate the LLD surface temperature to the measured influx of impurity and hydrogenic species.

II. METHOD

Plasma operations with evaporated lithium coatings in NSTX bring up a number of diagnostic concerns. The concerns include (1) degradation in transmission of diagnostic port windows and reflectivity of in-vessel mirrors due to exposure to lithium fluxes, (2) deposition of lithium on exposed diagnostic parts (e.g., foil filters, probe surfaces), and (3) large changes in the dynamic range of some measured quantities (e.g., edge neutral pressure,

n_e , recycling) due to lithium pumping. These concerns are generally addressed by diagnostic hardware modifications or additional calibration efforts.

Evaporated lithium coatings can also affect measurements directly: for example, reflections of light from the LLD surface can complicate the interpretation of the VIS and IR spectroscopy. To understand the impact of reflections, the reflectivities of common fusion PFCs (e.g., graphite, molybdenum) are characterized in the laboratory and incorporated in numerical diagnostic models^{7,8}. Reflectivities of lithium-coated PFCs, however, have not been studied. While laboratory data in this case may help interpret visible spectroscopic measurements from the LLD, the impact of a dynamic, real-time variation in the LLD surface conditions would still be a concern. In NSTX, lithium coatings evaporated on graphite PFCs tended to increase surface reflectivity, as was apparent in the VIS and IR camera measurements. The LLD module was designed to operate at temperatures up to 350° C, well above the lithium melting point 180° C. Liquid lithium has a mirror-like appearance with high reflectivity in the VIS range⁹. According to Ref.¹⁰ data, the reflectance of liquid lithium at normal incidence is 0.5-0.95 throughout the visible range, 0.3-0.5 in the UV range, and ≤ 0.01 in the far-UV range. This motivated us to consider spectroscopic measurements in the near and far UV range, where reflectivities are low.

Photometrically calibrated spectroscopy and the S/XB technique¹¹ will be used for plasma-LLD interaction analysis, measurements of recycling and impurity particle fluxes. The S/XB technique relates spectral line intensities to particle influx using the ionizations per photon factors S/XB (where S, X are the ionization and excitation rates and B is the branching ratio (a ratio of radiative transition probabilities) for the spectral line used) from collisional-radiative model calculations or laboratory measurements. The S/XB technique assumes that the ionization and excitation processes occur in a common plasma volume characterized by T_e and n_e . Independent local T_e and n_e measurements with, e.g., Langmuir probes, are therefore of high priority since the S/XB factors are generally T_e and n_e -dependent. Using the divertor ionization flux Γ_i^{out} inferred from the visible Balmer- α, β and far-UV Ly $_{\alpha}$ emission line intensities, and the ion flux incident on the divertor surface Γ_i^{in} from the Langmuir probes⁴, a local recycling coefficient $R = \Gamma_i^{out}/\Gamma_i^{in}$ can be estimated. This is particularly important for numerical modeling of the LLD experiments. The recycling coefficient R is presently used in 2D edge transport fluid codes as a free input parameter to model the impact of lithium on scrape-off layer (SOL) plasma transport¹². To assess PFC

TABLE I. Candidate spectral lines for divertor deuterium and impurity flux measurements in NSTX.

Species	Wavelength (nm)
D Balmer series	376.9, 379.7, 383.4, 388.8, 396.9, 410.0, 433.9, 486.0, 656.1
D ₂ $d^3\Pi_u - a^3\Pi_g^+$ Fulcher band	592 - 602
He I	388.9, 587.5, 667.8, 706.7, 1083.0
He II	320.3, 468.5, 541.1
Li I	323.3, 413.2, 460.3, 610.4, 670.8
Li II	319.9, 325.0, 467.8, 478.9, 548.5
LiD $A^1\Sigma^+ - X^1\Sigma^+$ band	330 - 470
Li ₂ $B^1\Pi_u - X^1\Sigma_g^+$ band	460 - 550
C I	493.2, 538.0, 833.5, 909.4, 1175.4
C II	392.0, 426.7, 514.0, 658.0, 678.0, 723.0
C III	407.0, 465.0, 569.6, 833.2, 850.0
C IV	465.8, 580.1
CD band $A^2\Delta - X^2\Pi$	431
CD band $B^2\Sigma - X^2\Pi$	390
Fe I	344.1, 358.1, 372.0, 649.5
Mo I	379.8, 386.4, 390.2, 550.6, 553.3, 557.0

impurity fluxes, the emission lines listed in Table I will be considered. For deuterium and main NSTX plasma impurities abundant S/XB data are available in the ADAS database¹³ and literature.

III. LYMAN α DIODE ARRAY

The objective of the LADA diagnostic is to measure neutral deuterium emission from the divertor region while minimizing parasitic contributions from reflections off the LLD module. For this reason, the deuterium Ly α $n = 2 - 1$ resonant line at $\lambda = 121.6$ nm (in the far UV) was selected. The measurements will be compared to those from the existing photometrically calibrated D $_{\alpha,\beta,\gamma}$ cameras¹⁴. The LADA diagnostic by its design is a filtered pinhole camera with a 1D array detector - an absolute AXUV silicon diode array from International Radiation Detectors, Inc. With proper handling and accurate accounting of the diagnostic factors (such as etendue, transmission, diode response, electronic gain factors), AXUV diode measurements are interpreted in absolute photometric units. A number of diagnostics based on AXUV diodes, including those for Ly α measurements, have been implemented on MCF

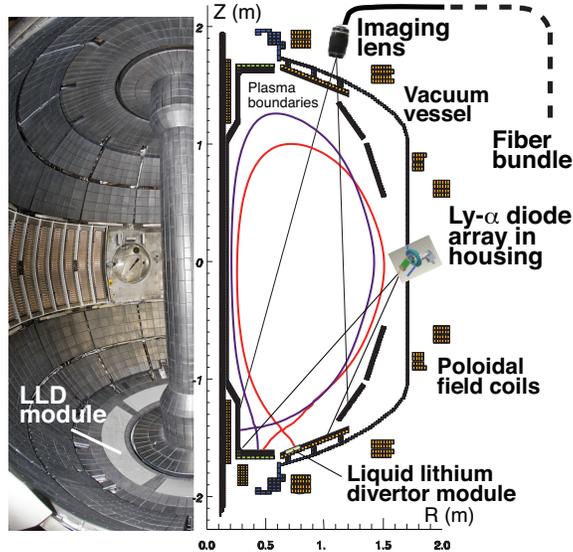


FIG. 1. Placement of the LADA and DIMS diagnostics on NSTX. Their divertor views are shown by thin lines.

plasma devices^{15–23}.

The LADA diagnostic is mounted on a 6” vacuum flange placed in the equatorial plane of the NSTX vacuum vessel (Fig. 1). The diagnostic layout is shown in Fig. 2. The in-vacuum diagnostic housing encloses a stainless steel block with a copper insert holding a precision slit disk and a spectral bandpass filter, and the diode array. The twenty element model AXUV20EL array is a compromise between the diode sensitive area (3 mm^2) and the diode element capacitance (nominally 1 nF) for an acceptable signal-to-noise ratio. The AXUV diode sensitivity is 0.11 A/W at $\lambda = 121.6 \text{ nm}$. The slit area is 2 mm^2 , and it is placed 10 cm from the diode array. Each diode element forms a monochromator with an etendue $\simeq 6 \times 10^{-10}$. For Ly_α spectral filtering, the open-faced filter Type 122-XN-.5D mounted on a 12.5 mm diameter MgF_2 substrate from Acton Research Corp. is used. The filter has a peak transmission 0.055 , and the measured bandpass (full width at half maximum - FWHM) 9.2 nm centered on the Ly_α line. No strong impurity lines are within the bandpass¹⁶, except the $\text{Li III } n = 6 - 3$ line at $\lambda = 121.6 \text{ nm}$ which is not expected to be strong in the divertor region. In order to keep the filter temperature at $T \leq 50 - 60^\circ \text{ C}$ during the NSTX vacuum vessel bake-out and LLD high-temperature operation, the stainless steel block with the copper insert and the filter are water-cooled. The cooling tubes are welded to the 6” mounting flange and form a loop inside the block. A remotely-controlled shutter is used

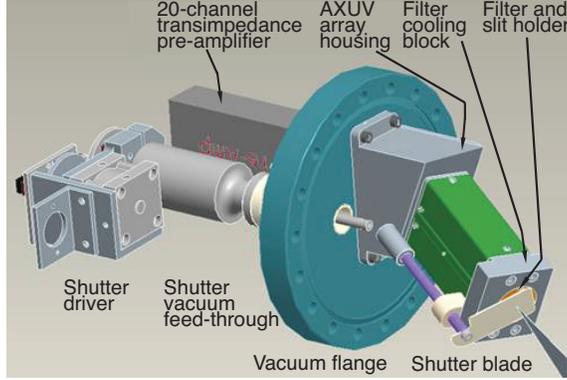


FIG. 2. Lyman- α diode array schematic.

to protect the slit and the filter from the line-of-sight lithium atoms evaporated from the LLD. The AXUV20EL array is connected to a pre-amplifier through a multi-pin DB-shell vacuum feedthrough. The twenty channel DC-coupled trans-impedance pre-amplifier Model 8986A built by Clear-Pulse, Inc. is mounted on the air side of the diagnostic. The pre-amplifier characteristics are: gain 10^6 , frequency response 10 kHz, output impedance 50Ω . A twisted-pair shielded cable is used to transmit analog signals to a ninety six channel digitizer module model ACQ196CPCI from D-TACQ Solutions Ltd. The digitizer module provides 16-bit digitization at 500 kSPS/channel and sends digital data directly to a MDS Plus server, eliminating a need for an additional PC.

The LADA diagnostic has been installed in NSTX and electronic background noise data in the range $\pm(10 - 40)$ mV has been recorded in initial NSTX 2010 campaign discharges. The thermal (Johnson) noise was estimated to be in the μV range. The expected Ly_α signals were estimated from the measured divertor D_α intensity and ADAS photon emission coefficients to be in the range 0.5 – 5 V.

IV. DIVERTOR IMAGING SPECTROMETER

The objective of the DIMS diagnostic is to provide *cm*-scale spatially resolved divertor profile measurements of 1) deuterium and impurity atomic and molecular emissions, and 2) divertor ion temperature T_i based on Doppler spectral line broadening. The term "imaging spectrometer" is used here to describe the concept of collecting light from several localized spatial regions in the divertor, relaying the light via separate fibers to the spectrometer en-

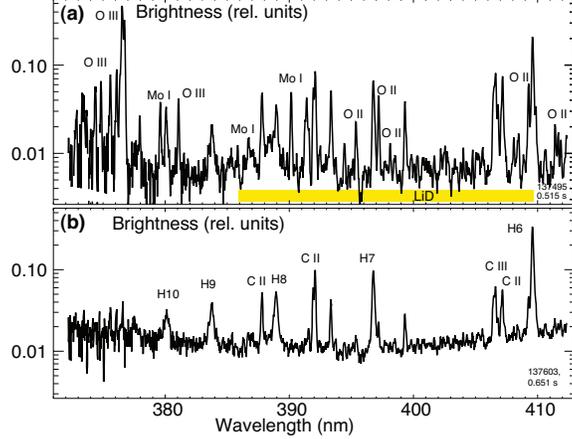


FIG. 3. UV spectra recorded from an LLD view by an existing divertor spectrometer in initial LLD experiments: (a) when a large MHD mode plasma hit the lower divertor; (b) with LLD at 320°C .

trance slit, and focusing the dispersed light on a 2D detector, while minimizing aberrations. Measurements by an existing 10-chord divertor imaging spectrometer²⁴ provided many important contributions to NSTX divertor studies^{24–27}, as well as insights for the design of the new system.

Particularly important for LLD protection will be operational monitoring of metal influx from the LLD. This will be accomplished by high spectral resolution measurements in the UV spectral region ($\leq 400\text{ nm}$). The presence of molybdenum (Mo I-II) or iron (Fe I-III) lines (e.g., Table I) in divertor spectra may be indicative of a direct plasma interaction with the LLD substrate and steel liner caused by insufficient lithium coating of the LLD surface. To illustrate this, Fig. 3 shows the UV spectra measured by the existing divertor spectrometer²⁴ with spectral resolution $\lambda/\delta\lambda \leq 4000$ in the initial LLD experiments. Molybdenum and iron lines were not measured routinely in discharges with the outer divertor strike point close to the LLD. In several discharges, the three Mo I lines (at 379.8, 386.4, and 390.2 nm) were identified in the fiber channel viewing the LLD module, following a large MHD event that impacted the cold ($T = 20 - 30^\circ\text{C}$) LLD. Also observed in the 380-410 nm range were molecular lines from the LiD band $A^1\Sigma_+ - X^1\Sigma_+$. In earlier NSTX experiments the CD B-X band and BD bands were observed in the same spectral range²⁴. Generally, these molecular band lines complicated atomic spectra interpretation. However, the molecular spectra can also contribute to understanding of LLD surface processes that depend on LLD temperature

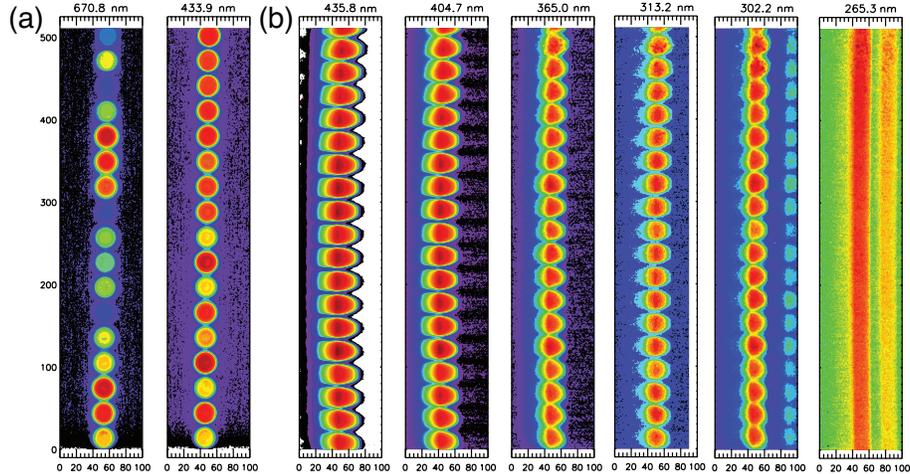


FIG. 4. (a) False-color images of input optics fibers focused with the DIMS achromatic triplets at $\lambda 670.8$ nm and $\lambda 433.9$ nm. Irregularities in fiber illumination were due to uneven source distribution; (b) Series of imaging UV spectra of Hg lines (wavelengths shown on top of each panel)

and surface conditions. A number of lithium deuteride, lithium carbonate, and lithium oxide compounds can form on the LLD surface affecting the reactions between ionized and neutral deuterium with lithium. For example, in 3 MW NBI-heated discharges with the LLD operated at $T \simeq 320^\circ$ C, a decrease in intensities of molecular and low Z impurity (C, O) lines was apparent, suggesting the clean-up of the LLD module surface (Fig. 3 (b)).

Nearly stigmatic, aberration-free, high spectral resolution imaging imposes challenging requirements on the diagnostic parameters and elements. The DIMS diagnostic has been designed as a system built from commercial components that maximize throughput yet minimize astigmatism and chromatic aberrations in a broad UV-VIS-NIR spectral range. The system consists of an imaging lens, a fiberoptic relay bundle, a spectrometer input fiber bundle, input imaging optics, and a spectrometer with a CCD detector. Each of these components was selected to provide good transmission, sensitivity, or achromatic imaging in a broad spectral range 200 - 1100 nm. In addition, the overall system etendue (system $F/\# = 4.7$) was optimized by matching $F/\#$ s of all individual components. Below we describe the DIMS in detail.

a. Divertor imaging and relay optics A six-element lens (model UV-105-4.5 Rayfact from Tochigi Nikon Inc.) with $f = 105$ mm, $F/\# = 4.5$ provides chromatically corrected

imaging and 0.70-0.80 transmission in the range 220-900 nm. The lens is mounted on a sapphire window port at a distance 3.4 m from the divertor surface (Fig. 1). The depth of field in the object plane is 10 - 20 cm thereby accommodating the variation in divertor shape. The acceptance angle $\gamma = 23.3^\circ$ enables a full view of the divertor with magnification $M \simeq 28$ and mm scale spatial resolution. A fiber array holder is mounted in the focal plane of the lens. The holder accommodates two parallel arrays of fibers: a new array of 48 silica-silica 400- μm diameter fibers from Polymicro, Inc. and an old array²⁴ of 24 quartz 600- μm diameter fibers from Fiberguide. Each 400- μm fiber collects light from a ~ 1 cm spot on the divertor. The UV-VIS-NIR transmission characteristics of the Polymicro Type FBP400440480 fibers in the 275 - 2100 nm range are superior to most available silica-silica high OH content fibers. The numerical aperture of each fiber is 0.22 ($F/\# = 2.27$). Both 30 m long fiber bundles relay light from the NSTX Test Cell to a remote radiation-shielded diagnostic room, where each fiber is terminated with an SMA-type connector.

b. Input optics and spectrometer In the diagnostic room, some of the relay fibers are coupled to the spectrometer input fiberoptic bundle via SMA connectors mounted in a switch-board box. The 4-meter long input fiber bundle consists of 20 fibers of the same Polymicro type. The bundle is terminated with a custom-made ferrule where the polished fiber ends form a linear array. The array is imaged 1:1 by the input optics on the entrance slit of the spectrometer. Two 30-mm diameter $F/\# = 2.0$ infinite-conjugate achromatic triplet lenses from Edmund Optics are used in the input optics assembly. The lenses are designed for a consistent (nearly constant) focal length in the spectral range 200 - 1000 nm. The spectrometer system consists of the McPherson, Inc. Model 207 $R = 0.67$ m Czerny-Turner monochromator and a CCD detector. The monochromator is equipped with large 120×140 mm gratings yielding the highest commercial $F/\# = 4.7$ for the focal length class. The Model 207 monochromator is also equipped with a master cylinder correcting mirror placed at the exit port to help correct imaging aberrations from spherical mirrors. Since the region of high-quality stigmatic imaging in the detector plane (in the dispersion direction) is limited, the extent of spectral domain on the CCD was not a priority. To provide high quality imaging and high CCD read out speed, we selected the Princeton Instruments camera Model Pro EM 512. The CCD camera has a square 512×512 chip with $16 \times 16 \mu\text{m}$ pixels. The back-illuminated e2v CCD97 chip based CCD camera incorporates the latest CCD technology features: an electron multiplication technology resulting in high quantum

efficiency and a frame-transfer architecture with an up to 10 MHz read out rate and 16-bit digitization. The CCD quantum efficiency in the UV range is enhanced by the Unichrome coating. A rack-mounted PC is used to control the monochromator wavelength drive via an RS-232 interface, and to read out the CCD camera data via a gigabit-ethernet cable using the Winspec software.

For high-resolution Doppler spectroscopy, three gratings with 3600, 2400, and 1800 gr/mm will be used. Nominal spectral resolution of the Model 207 monochromator with the 3600 (1800) gr/mm grating is 0.012 (0.020) nm, and the dispersion is 0.43 (0.83) nm/mm. Typically, 4 pixels per line is sufficient for a reliable Gaussian fit to the data, yielding 0.064 mm FWHM on the CCD as a minimum requirement for the instrumental function width. For the 3600 gr/mm grating, the instrumental FWHM is 0.028 nm, enabling sufficient resolution to measure, e.g., $T_i = 3 - 5$ eV of D and He atoms (ions), and $T_i = 5 - 10$ eV of Li and C atoms (ions). However, when a monochromator is used for imaging with a cylinder mirror, its resolution is slightly degraded. Spectral resolution tests of the DIMS diagnostic are underway and will be reported elsewhere.

c. Tests of imaging quality The DIMS diagnostic has been assembled as described above, and initial imaging tests showed excellent transmission and imaging properties of the DIMS system in the UV range. In Fig. 4 (a) the properties of the achromatic triplet lenses were tested. The input fiberoptic bundle was illuminated and the fibers were imaged on the CCD detector using the aligned triplets. A broadband LED source was used for illumination with two $\Delta\lambda = 1.0$ nm bandpass interference filters with central wavelengths at $\lambda 670.8$ nm and $\lambda 433.9$ nm. Fig. 4 (b) shows the results from initial spectral imaging tests that included the input optics, monochromator and CCD detector. In this test, a 3600 gr/mm grating was used in the McPherson monochromator with $d = 25$ μm slit, and a fluorescent lamp was used as a source of Hg lines $\lambda = 435.8, 404.7, 365.0, 313.2, 302.2$ nm (in the right-most panel a pen-ray Hg lamp was used in front of the monochromator slit to obtain $\lambda = 265.3$ nm).

In conclusion, two new divertor imaging diagnostics are being developed for the liquid lithium divertor characterization on NSTX: a Ly_α diode array, and an UV-VIS-NIR high-resolution spectrometer. These diagnostics will provide recycling and impurity particle flux measurements for the LLD protection and performance evaluation.

ACKNOWLEDGMENTS

The authors would like to thank J. Abramson, P. Sichta, G. Tchilinguirian, G. Zimmer, D. LaBrie, T. Holoman, and G. Smalley (PPPL) for computer and technical support. Drs. M. G. Bell, B. Stratton (PPPL) and K. Tritz (Johns Hopkins U.) are acknowledged for technical discussions. Entire NSTX Team is acknowledged for research, plasma, and neutral beam operations. This work was performed under the auspices of the U.S. Department of Energy under Contracts DE-AC52-07NA27344 and DE-AC02-09CH11466.

REFERENCES

- ¹H. Kugel, M. Bell, J.-W. Ahn, J. Allain, R. Bell, J. Boedo, C. Bush, D. Gates, T. Gray, S. Kaye, R. Kaita, B. LeBlanc, R. Maingi, R. Majeski, D. Mansfield, J. Menard, D. Mueller, M. Ono, S. Paul, R. Raman, A. Roquemore, P. Ross, S. Sabbagh, H. Schneider, C. Skinner, V. Soukhanovskii, T. Stevenson, J. Timberlake, W. Wampler, and L. Zakharov, *Phys. Plasmas*, **15**, 056118 (2008).
- ²M. Bell, H. Kugel, R. Kaita, L. Zakharov, H. Schneider, B. LeBlanc, D. Mansfield, R. Bell, R. Maingi, S. Ding, S. Kaye, S. Paul, S. Gerhardt, J. Canik, J. Hosea, and G. Taylor, *Plasma Phys. Control. Fusion*, **51**, 124054 (2009).
- ³H. Kugel, M. Bell, L. Berzak, A. Brooks, R. Ellis, S. Gerhardt, H. Harjes, R. Kaita, J. Kallman, R. Maingi, R. Majeski, D. Mansfield, J. Menard, R. Nygren, V. Soukhanovskii, D. Stotler, P. Wakeland, and L. Zakharov, *Fusion Eng. Des.*, **84**, 1125 (2009).
- ⁴J. Kallman and M. Jaworski, *These proceedings* (2010).
- ⁵A. McLean, *These proceedings* (2010).
- ⁶R. E. Bell, *These proceedings* (2010).
- ⁷E. M. Hollmann, A. Y. Pigarov, and R. P. Doerner, *Rev. Sci. Instrum.*, **74**, 3984 (2003).
- ⁸K.-D. Zastrow, S. R. Keatings, L. Marot, M. G. O'Mullane, G. de Temmerman, and J.-E. Contributors, *Rev. Sci. Instrum.*, **79**, 10F527 (2008).
- ⁹R. Kaita, R. Majeski, R. Doerner, T. Gray, H. Kugel, T. Lynch, R. Maingi, D. Mansfield, V. Soukhanovskii, J. Spaleta, J. Timberlake, and L. Zakharov, *J. Nucl. Mater.*, **363-365**, 1231 (2007).
- ¹⁰M. Rasigni and G. Rasigni, *J. Opt. Soc. Am.*, **67**, 54 (1977).

- ¹¹K. Behringer, *J. Nucl. Mater.*, **145-147**, 145 (1987).
- ¹²R. D. Smirnov, A. Y. Pigarov, S. I. Krasheninnikov, T. D. Rognlien, V. A. Soukhanovskii, M. E. Rensink, R. Maingi, C. H. Skinner, D. P. Stotler, R. E. Bell, and H. W. Kugel, *Contrib. Plasma Physics*, **50**, 299 (2010).
- ¹³H. P. Summers, The ADAS User Manual, version 2.6, <http://adas.phys.strath.ac.uk> (2004).
- ¹⁴V. Soukhanovskii, A. Roquemore, C. Skinner, J. Menard, H. Kugel, D. Johnson, R. Maingi, S. Sabbagh, and F. Paoletti, *Rev. Sci. Instrum.*, **74**, 2094 (2003).
- ¹⁵I. Fumo, H. Weisen, J. Mlynar, R. Pitts, X. Llobet, P. Marmillod, and G. Pochon, *Rev. Sci. Instrum.*, **70**, 4552 (1999).
- ¹⁶R. Boivin, J. Goetz, E. Marmar, J. Rice, and J. Terry, *Rev. Sci. Instrum.*, **70**, 260 (1999).
- ¹⁷D. Stutman, M. Finkenthal, V. Soukhanovskii, M. May, H. Moos, and R. Kaita, *Rev. Sci. Instrum.*, **70**, 572 (1999).
- ¹⁸V. Soukhanovskii, D. Stutman, M. Iovea, M. Finkenthal, H. Moos, T. Munsat, B. Jones, D. Hoffman, R. Kaita, and R. Majeski, *Rev. Sci. Instrum.*, **72**, 737 (2001).
- ¹⁹D. Gray, S. Luckhardt, L. Chousal, G. Gunner, A. Kellman, and D. Whyte, *Rev. Sci. Instrum.*, **75**, 376 (2004).
- ²⁰A. Degeling, H. Weisen, A. Zabolotsky, B. Duval, R. Pitts, M. Wischmeier, P. Lavanchy, P. Marmillod, and G. Pochon, *Rev. Sci. Instrum.*, **75**, 4139 (2004).
- ²¹C. Suzuki, B. Peterson, and K. Ida, *Rev. Sci. Instrum.*, **75**, 4142 (2004).
- ²²M. Reinke and I. Hutchinson, *Rev. Sci. Instrum.*, **79**, 10 (2008).
- ²³E. Granstedt, These proceedings (2010).
- ²⁴V. Soukhanovskii, D. Johnson, R. Kaita, and A. Roquemore, *Rev. Sci. Instrum.*, **77**, 10127 (2006).
- ²⁵V. Soukhanovskii, *Rev. Sci. Instrum.*, **79**, 10F539 (2008).
- ²⁶V. Soukhanovskii, R. Maingi, D. Gates, J. Menard, S. Paul, R. Raman, A. Roquemore, M. Bell, R. Bell, J. Boedo, C. Bush, R. Kaita, H. Kugel, B. LeBlanc, and D. Mueller, *Phys. Plasmas*, **16**, 022501 (2009).
- ²⁷V. Soukhanovskii, R. Maingi, D. Gates, J. Menard, S. Paul, R. Raman, A. Roquemore, R. Bell, C. Bush, R. Kaita, H. Kugel, B. LeBlanc, and D. Mueller, *Nucl. Fusion*, **49**, 095025 (2009).